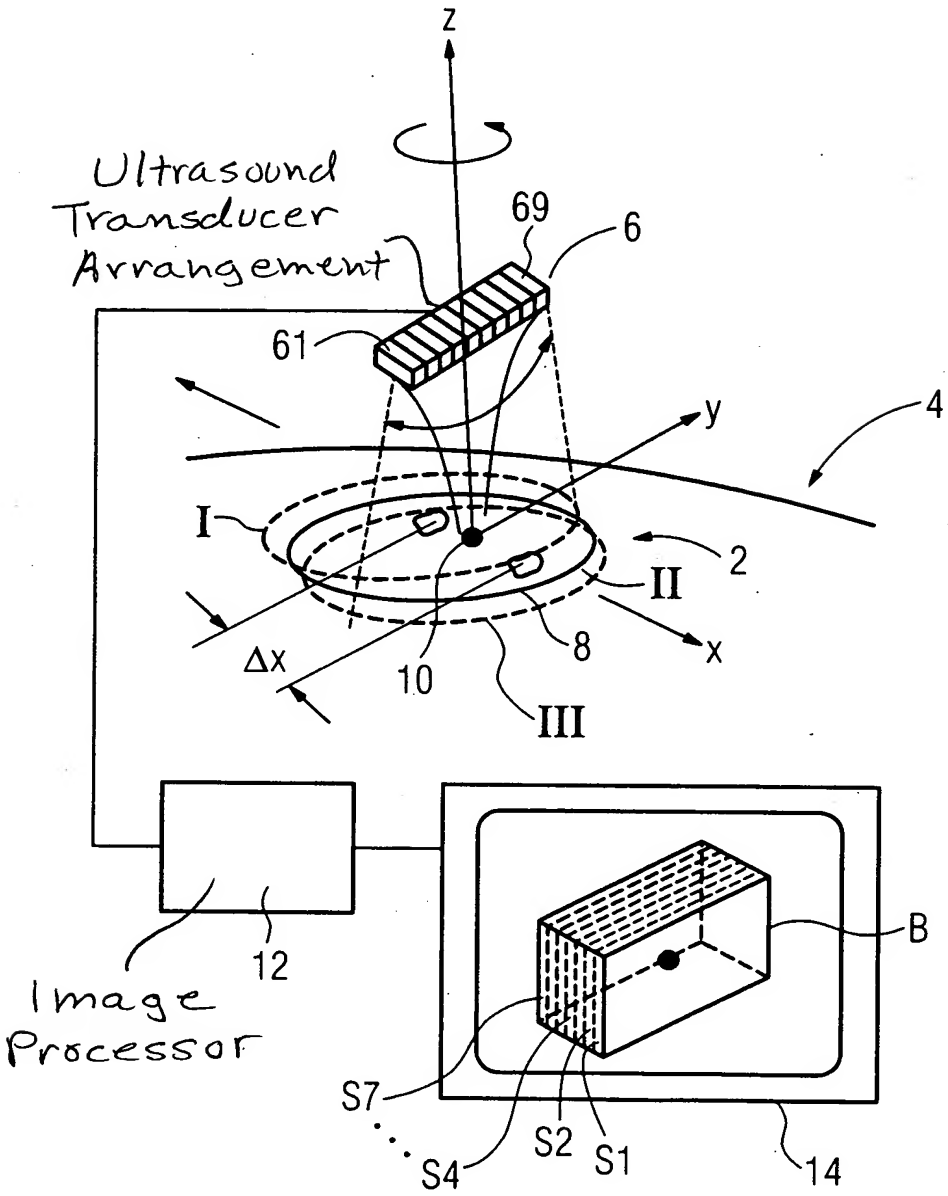
z
Ultrasound Transducer Arrangement
69
6
61
y
4
I
2
II
8
x
Δx
10
III
12
Image Processor
B
S7
S4
S2
S1
14